

Location Test Lab CMTF 2 <sup>nd</sup> Floor	Accelerator Operating Conditions	Instrument: _____ Serial #: _____ Calibration due: _____	RWP
---	----------------------------------	--	-----

Reason for survey:

- LEGEND**  
All readings in mR/h whole body (unless annotated otherwise)
- Denotes posted area
  - Ⓝ Denotes smear location (results attached if applicable)
  - ☐# Denotes tritium wipe/swab (results attached if applicable)
  - Contact dose rate
  - 30 cm dose rate
  - Item description
  - ↓
  - ▨ Denotes area not surveyed

- Abbreviations**
- RMA – radioactive material area
  - RCA – radiologically controlled area
  - RA – radiation area
  - HRA – high radiation area
  - CA – contamination area
  - HCA – high contamination area


**Beam Enclosure Entry Surveys**

Full survey, all areas posted

Partial survey with continuous surveillance

N/A

Comments:

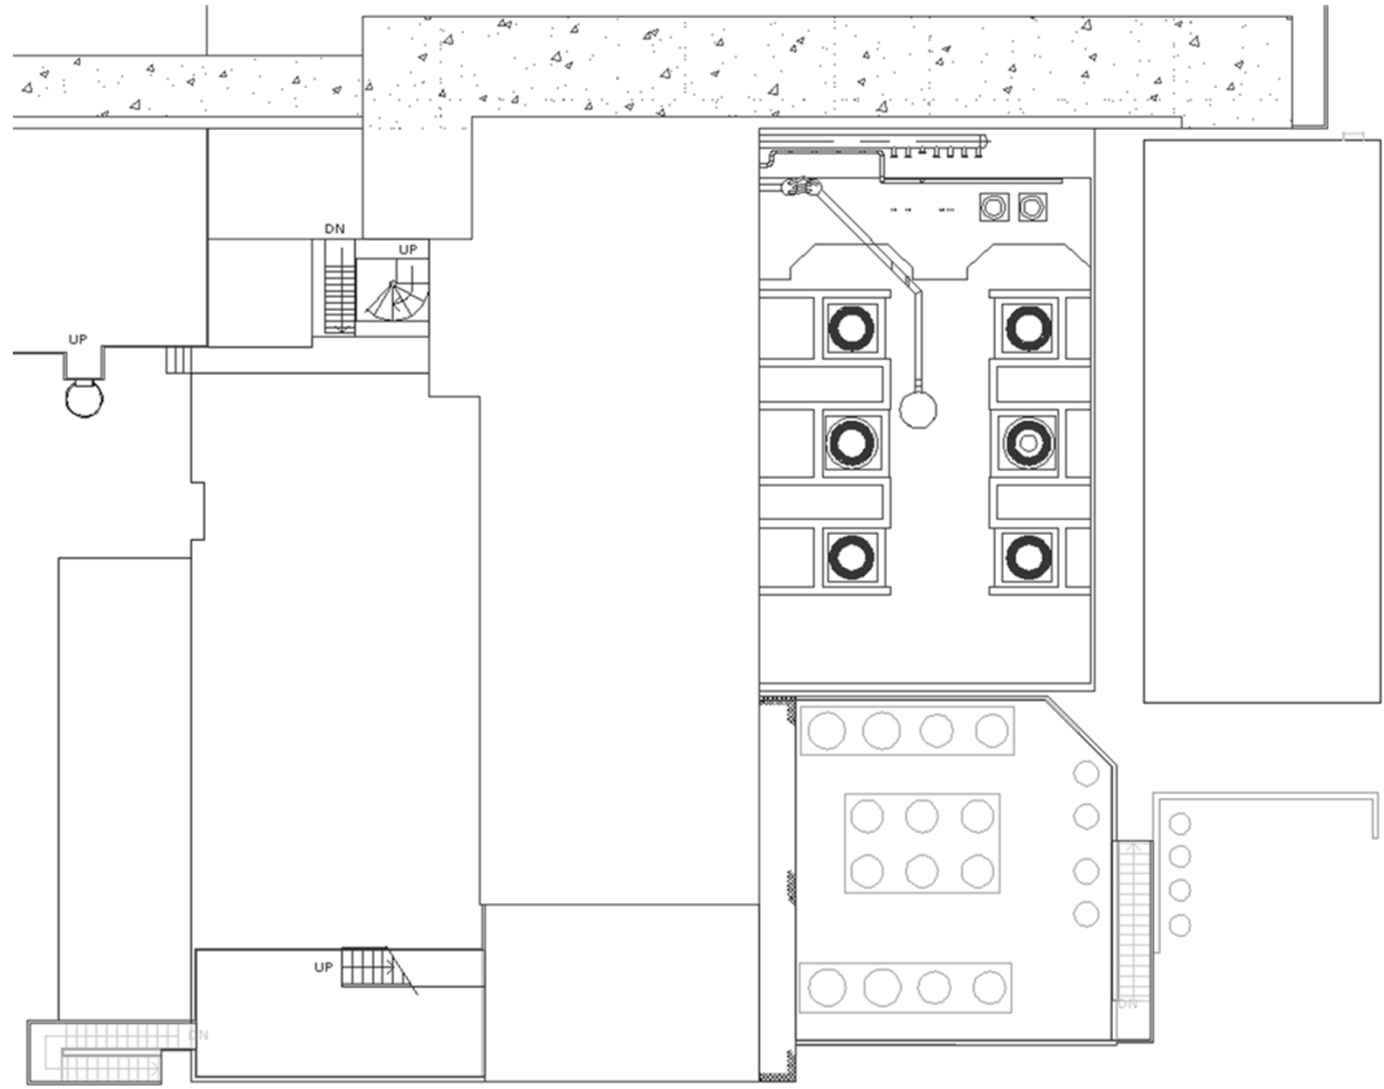

Performed by (print)	Date / /	Crew Chief Review (print)	Date / /	RCD Review (print)	Date
Sign	Time	Sign	Time	Sign	/ /